



**OPTIS™ Mobile Next**  
**Imaging System**



**REF** 1014932

**Operation and Maintenance Manual**



# Contents

Symbols .....	1
OPTIS™ Mobile Next Imaging System .....	5
Safety Information .....	6
Patient Safety .....	6
Operator Safety .....	8
Moving the System.....	9
Avoiding Electrical Hazards.....	10
Electromagnetic Interference .....	12
Safety Functions Built Into the OPTIS Mobile Next .....	13
Indications for Use .....	14
Contraindications .....	14
Complications.....	15
Warnings and Precautions.....	15
Warnings.....	15
Warnings (OCT) .....	15
Precautions (OCT) .....	16
Warnings and Precautions (Fractional Flow Reserve [FFR], Resting Full-Cycle Ratio [RFR]) .....	17
Connecting to External Equipment / Accessories .....	17
Mechanical Enclosure .....	18
Electrical.....	18
Electronic Interference.....	19
Aortic Reference Pressure.....	19
Defibrillation.....	19
System Security .....	19
System Overview .....	20
System Features.....	20
System Components.....	21
System Setup .....	27
Positioning the System.....	27
Attaching and Removing Components (Table Rail) .....	28
Connecting the System .....	29
Powering On.....	32
Shutting Down.....	32
Cleaning and Maintenance .....	33
Cleaning .....	33
Maintenance .....	34
Infection Control .....	39
User Troubleshooting .....	40
System Disposal .....	41
System Specifications.....	42
System - Safety and Regulatory.....	42
System - Electrical and Physical.....	43
Imaging Specifications .....	44
Physiology Specifications .....	44
Electromagnetic Emissions .....	45
Electromagnetic Immunity.....	45
Recommended Separation Distances .....	47
FCC Statement.....	48
Essential Performance.....	48



## Symbols

The following symbols may be found on the product or product label:

Symbol	Definition
	Equipotentiality
	For indoor use only
IPX3	Protection from a spray of water in any direction when the device is up to 60° any direction from vertical for at least 5 minutes.
	Bureau Veritas (Nationally Recognized Test Laboratory)
	Warning; laser beam
	Video Out
	Video In
	Network
	Universal serial bus port/plug
	No pushing
	Japan Technical Conformity Mark Japanese RF identifier for the transmitter.
	Australian Communications and Media Authority (ACMA) and New Zealand Radio Spectrum Management (RSM) Regulatory Compliance Mark (RCM)
R-NZ	New Zealand Radio Spectrum Management (RSM) compliance mark for products that have radio transmitters of conformity level A1, A2, or A3
	KCC identifier
	FCC Identifier
IC:	IC identifier for transmitter  This device complies with RSS-210 of the IC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation

## Symbols (continued)

Symbol	Definition
	Separate collection for waste electrical / electronic equipment.
	Mass; weight
	Fuse
	Software
	Unique device identifier
	Medical device
	Manufacturer
	Consult instructions for use
	Caution
	Do not use if package is damaged
	Keep dry
	Humidity limitation
	Temperature limit
	Packaging unit

## Symbols (continued)

Symbol	Definition
	Date of manufacture
	Catalogue number
	Serial number
	Non-ionizing electromagnetic radiation
	Japan Ministry of Internal Affairs and Communications High Frequency Mark
	Refer to instruction manual/booklet
	Symbol with certification number denotes radio type approval for Brazil by Agência Nacional de Telecomunicações (Anatel)
	Defibrillation-proof type CF applied part
	Authorized representative in the European Community



## OPTIS™ Mobile Next Imaging System

### About This Manual

This manual describes the Abbott Medical OPTIS Mobile Next system and accessories. It provides information on:

- Safety and risk statements
- System components
- Cleaning and maintenance
- Specifications

Pictures shown are for example only.

#### Note:

- For a full description of Optical Coherence Tomography (OCT) and physiology procedures, including a list of compatible Dragonfly™ Imaging Catheters, refer to the installed software User Manual.
- Details of the imaging catheter are covered in the Dragonfly Imaging Catheter Instructions for Use provided with the catheter and are not covered in this manual.
- Details of the PressureWire™ X Guidewire and the PressureWire™ Aeris™ FFR Measurement System with Agile Tip Technology are covered in the Instructions for Use provided with these items, and are not covered in this manual.
- Refer to the Wi-Box™ AO Transmitter Instructions for Use for set-up procedures for the Wi-Box AO Transmitter.
- This manual does not provide detailed discussion of system components, except as they are used with the OPTIS Mobile Next.

## Safety Information

---



**CAUTION:** Before using the OPTIS™ Mobile Next for the first time, be sure to read and understand all of the information in this chapter. Carefully read all instructions prior to use. Observe all warnings and precautions noted throughout these instructions; otherwise, complications may occur.

---

Although the OPTIS Mobile Next conforms to laser emission standards and both international and European safety and electromagnetic compatibility standards, the system is intended for use only by medical personnel who are knowledgeable in OCT and physiology procedures. Only a knowledgeable operator can determine if OPTIS Mobile Next use is appropriate. An awareness of system limitations is essential to making that determination and ensuring safe operation for both operator and patient.

This section provides information on:

- Patient safety
- Operator safety
- Moving the system
- Avoiding electrical hazards
- Electromagnetic interference
- Built-in safety functions

### Patient Safety

The OPTIS Mobile Next is intended for use only by medical personnel who are familiar with its operation and skilled in the clinical procedures to be used.

To avoid any potential hazard to patients, follow the precautions outlined in this section.



**CAUTION:** Use only the compatible Dragonfly™ Imaging Catheter with the OPTIS Mobile Next. Use of other types of catheters may result in unsafe conditions for the patient and damage the OPTIS Mobile Next.

---

---

## General

---



**WARNING:** Failure to follow the guidelines described in these Instructions for Use and in the Instructions for Use provided with the accessories may result in injury to patients and damage to equipment.

---



**WARNING:** Failure to abide by the precautions detailed below causes the system and its use to be out of compliance with regulations and places the patient and the operator at risk of injury or death.

---



**WARNING:** Connecting to External Equipment / Accessories - When used in the patient environment, all equipment connected to the OPTIS Mobile Next must meet the requirements for medical isolation according to the IEC 60601 safety standards. Connection of equipment that does not follow relevant IEC standards (e.g., IEC 60601 series for medical electrical equipment) may lead to patient injury or death.

---



**WARNING:** Electrical Shock Hazard - Do not remove OPTIS Mobile Next covers. To avoid electrical shock, use only the power cord supplied with the system and connect only to properly grounded wall outlets. Refer to “System Setup” and “Safety Information” for electrical safety information.

---



**WARNING:** The Dragonfly Imaging Catheter is sterilized by ethylene oxide and is intended for one-time use only. Non-pyrogenic. Do not use if the package is opened or damaged. Do not reuse or re-sterilize. Any attempt to reuse or re-sterilize may compromise the structural integrity of this device. Adverse effects of using a non-sterile or re-sterilized catheter may include, but are not limited to: local and / or systemic infection, mechanical damage, inaccurate results.

---



**WARNING:** Do not use the PressureWire™ Guidewire if there are any signs of damage.

---



**CAUTION:** Please note Abbott Medical makes no representation or warranty that use of the OPTIS Mobile Next complies with applicable privacy, security, and confidentiality laws, but encourages you to assess your own risk as you use, disclose, control, process, or transfer patient health information with the OPTIS Mobile Next.

---

- Use only compatible Dragonfly Imaging Catheters. Always use under appropriate imaging guidance (endoscopy, x-ray fluoroscopy, or other appropriate guidance method).

## Safety Information

---

- Use only compatible wireless PressureWire Guidewires to report aortic distal pressure. Always use under appropriate imaging guidance (endoscopy, x-ray fluoroscopy, or other appropriate guidance method).
- Always read and follow the Instructions for Use supplied with the Dragonfly Imaging Catheter and with the PressureWire Guidewire.
- Always use controls, make adjustments, and perform procedures as specified in these Instructions for Use.

### Techniques to Minimize Patient Exposure

The OPTIS Mobile Next meets the performance standards of laser-emitting products as established by IEC 60825-1. Although no harmful effects have been demonstrated for the near-infrared light wavelengths, intensities, and exposure times used during examinations with the OPTIS Mobile Next, Abbott Medical recommends that you carefully read the warning labels on the system (refer to “Avoiding Operator Light Emission Hazards” [page 8]) and follow these examination guidelines:

- Use OCT only when there is a good reason to do so.
- Use techniques that enable quick collection of clinical data and shorten procedure time.

### Operator Safety

#### Avoiding Operator Light Emission Hazards

To avoid any potential light emission hazards to you or to patients, adhere to the information provided in the safety labels that are located on the system (figure below) and observe the precautions outlined in this section.




---

**WARNING:** Failure to follow any of these precautions may cause possible serious damage to your eyes.

---

Figure 1. Connector Panel Laser Safety Label



- Avoid eye exposure. Do not look at or stare directly into the beam. Doing so may damage your eyes.




---

**WARNING:** Viewing the laser output with telescopic optical instruments (e.g., telescopes and binoculars) may pose an eye hazard and thus the user should not direct the beam into an area where such instruments are likely to be used.

---

- Use controls, make adjustments, and perform procedures only as specified in these Instructions for Use.

### Repetitive Strain Injury (RSI)

Repetitive use of a mouse and keyboard has been associated with Carpal Tunnel Syndrome (CTS) and related musculoskeletal problems. Follow these suggestions to help prevent these problems:

- Maintain your joints in optimum positions with a balanced posture, avoiding:
  - Static postures
  - Exertion of force during repetitive motions
  - Wrist flexion or deviation
- Position the keyboard and monitor to minimize reaching and stretching.
- Take frequent breaks to give tissues time to recuperate from awkward positions and repetitive movements.

### Moving the System

When moving the system, observe these precautions:



---

**WARNING:** Failure to position the system as described may lead to a system tipping hazard or a pinching hazard, causing possible patient or operator injury and damage to the system.

---

- Be sure to turn off the system and disconnect all cables (video in, video out, Ethernet, and power cord) before beginning a move.
- Place the drive motor and optical controller (DOC) cable in the storage tray and secure the cable with the cord hook. Before storing the DOC, close the dust cover.
- Move the system using the grab bars on the work surface.
  - Do not use the DOC cables or video cables to move the system.
  - Do not pinch or excessively bend the cables while moving the system.
- The system weighs up to 80 kg (176 lbs) with all accessories installed.
- Make sure that the system wheels roll freely before beginning the move. Resolve any wheel problems before you move the system.

**Note:** Be sure the system brakes are in the up position (unlocked).
- To eliminate the potential danger of the system tipping over, avoid ramps that are steeper than 5 degrees.
- Do not push the system by the monitors or monitor support mount.
- If you must move the system up or down ramps with an incline of more than 5 degrees, use two people.

**Note:** Wheelchair ramps usually have an incline of less than 5 degrees.
- Do not lift a cart bearing the system to move it over uneven elevator entrances or other steps and barriers. Use a route that avoids such problems.

## Safety Information

---

- When using a transport vehicle, be sure that it can handle the weight of the system components plus passengers.
- If a lift is used, be sure the load capacity of the lift can accommodate the weight of the system components plus passengers.

### Avoiding Electrical Hazards

---



**WARNING:** To maintain compliance with regulatory standards, all components supplied with the system or specified as part of the system are to be powered by power supplies and power cords provided with the system. No unauthorized substitutions are permitted.

---

When transferring files inside the catheterization laboratory, use only port-powered USB drives.



**WARNING:** Inside the catheterization laboratory only port-powered USB drives may be connected to the USB port. Connecting externally powered devices to the USB port in the patient vicinity may compromise electrical isolation and cause patient injury.

---

**Note:** Outside the catheterization laboratory, IEC 60950-compliant, externally powered USB hard drives may be connected to the USB port.

Do not remove system covers. Only qualified personnel should service the system. Accidentally contacting the electrical circuits inside the housing could cause serious injury.

## Making Proper Electrical Connections

Ensure that the electrical connection for the system is properly rated (figure below). Carefully follow the safety guidelines described in this section when connecting the system power cord to the hospital or laboratory AC outlet.




**WARNING:** Failure to follow the electrical connection precautions detailed in this section causes the system and its use to be out of compliance with regulations and places the patient and the operator at risk of injury or death, and may damage the equipment.



**WARNING:** Do not allow the tableside controller (TSC) power supply to get wet.

Figure 2. Electrical Label

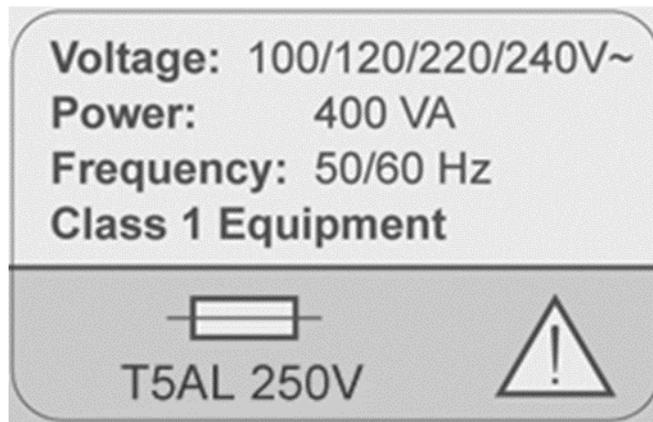

- Connect the system only to properly grounded (three-hole) hospital-grade AC outlets:
  - The circuit must accommodate an additional load of up to 400 VA.
- Replacement fuses are available through Abbott Medical.
- The power cord is to be used for disconnection from main power.
- Make sure any devices that connect to the network interface of the OPTIS Mobile Next comply with the appropriate IEC / national standard and are certified to IEC 60950.
- Use no electrical peripherals within 6 feet (1.83 m) of a patient unless the peripherals receive power from an isolation transformer that meets medical safety standards.

**Note:** If the OPTIS Mobile Next is used with peripherals that are powered from a separate wall outlet, the combination is considered to be a Medical System. It is the user's responsibility to comply with IEC 60601-1 and test the Medical System according to the requirements.

## Safety Information

---

### Explosion Hazard



**WARNING:** Do not operate the OPTIS Mobile Next in the presence of flammable anesthetics. Doing so could lead to an explosion.

---

### System Imaging Limitations

The OPTIS Mobile Next is intended for use by medical personnel who are knowledgeable in OCT and Physiology procedures. To determine if system use is appropriate, the user must be aware of system imaging limitations.

### Considerations for Optimal Vessel Imaging

The OPTIS Mobile Next can be used to image through vessels or to image the inner surface of certain vessels. Because the Dragonfly Imaging Catheter is smaller than the diameter of the vessel being imaged, the position of the catheter in the vessel has an effect on the portion of the vessel that can be imaged.

- Imaging range is greatest when the Imaging Catheter is centered in the lumen.
- Imaging range is least when the Imaging Catheter is placed off-center in the lumen, against the wall of the vessel.

### Considerations for Optimal Tissue Imaging

The maximum imaging depth within a vessel wall ranges from approximately 0.9 mm to 1.3 mm and is limited by optical attenuation caused by scattering of the optical beam by microstructures in the vessel. For example, penetration of the OCT beam is deepest in calcified tissue and shallowest in dense fibrotic tissue.

### Electromagnetic Interference

The system produces images by using digital signal processing techniques that operate in the radio frequency (RF) energy range. The system is therefore susceptible to interference generated by other RF energy sources such as medical devices, information technology products, or radio / television transmission towers. Tracing the source of radiated interference can be difficult.

The user must determine if an artifact caused by radiated interference will negatively impact image quality and the subsequent study results.

To help identify the source of electromagnetic interference, ask the following questions:

- Is the interference intermittent or constant?
- Does the interference occur with one catheter only, or with other imaging catheters?

- Is the interference present if the system is moved to a different location in the facility? Examples: Placing the system close to an ECG cable can increase electromagnetic interference. Moving the cable or other medical equipment away from the system can reduce electromagnetic interference.

Please answer these questions before contacting Abbott Service. The answers will help determine if the problem is in the system or in the imaging environment.

### **Safety Functions Built Into the OPTIS Mobile Next**

The following safety functions have been built into the system:

- The system disables light output and disables all motors in these situations:
  - The optical fiber stops rotating due to mechanical failure.
  - Communication is lost between the imaging engine and the DOC.
  - Communication is lost between the computer and the imaging engine.
- Pressing the Stop button on the DOC disables power to the DOC and laser output. Refer to “Drive Motor and Optical Controller (DOC)” on page 25.

## Indications for Use

The OPTIS™ Mobile Next with a compatible Dragonfly™ OPTIS™ or Dragonfly OpStar™ Imaging Catheter is indicated for:

- For qualitative and quantitative evaluation of vascular morphology in the coronary arteries
- As an adjunct to conventional angiographic procedure to provide an image of vessel lumen and wall structures
- For imaging of coronary arteries and is indicated in patients who are candidates for transluminal interventional procedure

The system further computes and displays various physiological parameters based on the output from one or more electrodes, transducers, or measuring devices.



---

**CAUTION:** The OPTIS Mobile Next is intended for use by medical personnel who are knowledgeable in OCT and physiological procedures. Abbott Medical and its employees cannot give instructions in the interpretation or diagnosis of recordings and makes no attempt to do so.

---



---

**CAUTION:** All operators must be knowledgeable in performing OCT and physiological procedures prior to using the installed software, OPTIS Mobile Next, and the Dragonfly Imaging Catheter.

---

## Contraindications

Use of the OPTIS™ Mobile Next is contraindicated where introduction of any catheter would constitute a threat to patient safety.

Contraindications include:

- Bacteremia or sepsis
- Major coagulation system abnormalities
- Patients diagnosed with coronary artery spasm
- Patients disqualified for coronary artery bypass graft (CABG) surgery
- Patients disqualified for percutaneous transluminal coronary angioplasty (PTCA)
- Severe hemodynamic instability or shock
- Total occlusion
- Large thrombus
- Acute renal failure
- Inability to tolerate systemic anticoagulation is a contraindication to use of OCT for coronary imaging.
- PressureWire™ Guidewire is contraindicated for use in the cerebral vasculature.
- The system has no patient alarm functions. Do not use for cardiac monitoring.

## Complications

The risks involved in vascular imaging include those associated with all catheterization procedures. The following complications may occur as a consequence of intravascular imaging and may necessitate additional medical treatment including surgical intervention.

- Abnormal heart rhythm or arrhythmias
- Acute myocardial infarction
- Allergic reaction to the contrast media or drug administered for the procedure
- Arterial dissection, injury, or perforation
- Bleeding
- Catheter access site reactions: sterile inflammation or granuloma
- Coronary artery spasm
- Death
- Embolism
- Myocardial ischemia
- Renal insufficiency or failure from contrast media use
- Repeat revascularization
- Thrombus formation, abrupt closure, or total occlusion
- Tissue necrosis
- Unstable angina
- Hypotension

## Warnings and Precautions

### Warnings

- Prior to use, please review the installed software User Manual and the Instructions for Use supplied with the OPTIS™ Mobile Next, Dragonfly™ Imaging Catheter, Wi-Box™ AO Transmitter, and PressureWire™ Guidewire for more information on warnings, limitations, cautions, and setup instructions.
- Leave the guide wire engaged with the Dragonfly Imaging Catheter at all times during use. Do not withdraw or advance the guide wire prior to withdrawing the Dragonfly Imaging Catheter.

### Warnings (OCT)

- Appropriate anticoagulant and vasodilator therapy must be used during the procedure as needed.

## Warnings and Precautions

---

- Observe all advancement and movement of the Dragonfly Imaging Catheter under fluoroscopy. Always advance and withdraw the catheter slowly. Failure to observe device movement fluoroscopically may result in vessel injury or device damage. To ensure proper placement, do not move the guide wire after the Dragonfly Imaging Catheter is in place.
- If resistance is encountered during advancement or withdrawal of the Dragonfly Imaging Catheter, stop manipulation and evaluate under fluoroscopy. If the cause of resistance cannot be determined or mitigated, carefully remove the Dragonfly Imaging Catheter and guide wire as a unit from the patient.
- The Dragonfly Imaging Catheter should never be forced into lumens that are narrower than the Dragonfly Imaging Catheter body or forced through a tight or heavily calcified lesion.
- The Dragonfly Imaging Catheter should not be advanced through abnormally tortuous anatomy.
- When advancing or retracting a Dragonfly Imaging Catheter with a monorail tip through a stented vessel, the Dragonfly Imaging Catheter may engage the stent between the junction of the Dragonfly Imaging Catheter and guide wire, resulting in entrapment of catheter / guide wire, catheter tip separation, stent dislocation, and / or vascular injury.
- Refer to the contrast media Instructions for Use for general warnings and precautions relating to use of contrast media.
- Before creating an OCT recording, review the installed software User Manual for additional warnings and cautions.

### Precautions (OCT)

- Follow all instructions, warnings, and cautions provided in “Patient Safety” on page 6 and in “Operator Safety” on page 8.
- Protect the exposed connector inside the DOC from fluids at all times. Fluid contact can disable the DOC and require service.
- For optimal imaging, only use 100% contrast media.
- When using saline, heparinized saline is recommended.
- Use the minimum flush rate and volume required to image the desired anatomy.
- Never attempt to attach or detach a Dragonfly Imaging Catheter to the DOC while the "lock" LED is lit.
- Do not kink, sharply bend, pinch, or crush the Dragonfly Imaging Catheter at any time.
- After use, the Dragonfly Imaging Catheter may be a potential biohazard. Handle and dispose of in accordance with accepted medical practice and applicable laws and regulations.
- The Dragonfly Imaging Catheter has no user serviceable parts. Do not attempt to repair or alter any part of the catheter assembly as provided.

## **Warnings and Precautions (Fractional Flow Reserve [FFR], Resting Full-Cycle Ratio [RFR])**

### **WARNING:**

- The PressureWire Guidewire is sterilized by ethylene oxide and is intended for one-time use only. Non-pyrogenic. Do not use if the package is opened or damaged. Do not reuse or re-sterilize. Any attempt to reuse or re-sterilize the PressureWire Guidewire may compromise the structural integrity of this device. Adverse effects of using a non-sterile or re-sterilized guide wire may include, but are not limited to: local and / or systemic infection, mechanical damage, inaccurate results.

### **CAUTION:**

- Patients with potential microvascular dysfunction and borderline index values should be interpreted with caution, and management strategies should be guided not only by pressure measurement, but also by possibly supplementary clinical risk stratification and other tests.
- Before performing a physiological parameter procedure, review the installed software User Manual for additional warnings and cautions.
- After use, the PressureWire Guidewire may be a potential biohazard. Handle and dispose of in accordance with accepted medical practice and applicable laws and regulations.
- The system may place the point of index value at the wrong location due to abnormal heart beat or artifact in Pa from flushing the guiding catheter. The responsible physician should confirm that the point selected by the system is a valid point of index value.
- If the cursor position has been saved, the index value is changed accordingly.
- Before creating a physiological parameter recording, review the installed software User Manual for additional warnings and cautions.

## **Connecting to External Equipment / Accessories**

### **WARNING:**

- When used in the patient environment, all equipment connected to the OPTIS Mobile Next must meet the requirements for medical isolation according to the IEC 60601 safety standards. Connection of equipment that does not follow relevant IEC standards (e.g., IEC 60601 series for medical electrical equipment) may lead to patient injury or death.
- Inside the catheterization laboratory only port-powered USB drives may be connected to the USB port. Connecting externally powered devices to the USB port in the patient vicinity may compromise electrical isolation and cause patient injury.

## Warnings and Precautions

---

### **CAUTION:**

- No connections to other systems or components are to be made to the OPTIS Mobile Next except through the Connector Panel. No connections are to be made through the Connector Panel except as described in this manual. In addition, all such combinations of systems shall comply with the standard IEC 60601-1, Medical electrical equipment - Part 1: General requirements for basic safety and essential performance. Any person who connects external equipment to the OPTIS Mobile Next has formed a medical system and is therefore responsible for compliance of the system with the requirements of IEC 60601-1. If in doubt contact a qualified technician. Only the PressureWire Guidewire and the Wi-Box AO Transmitter are intended to be used with the OPTIS Mobile Next wireless receivers.
- To connect to the correct Wi-Box AO Transmitter, you must select the room where the system is being used. The first time you connect to a room, you must enter the room's information into the system. Refer to the installed software User Manual for more information.

### **Mechanical Enclosure**

#### **WARNING:**

- Do not use the OPTIS Mobile Next if it has been dropped or in another way exposed to mechanical or electrical damage or if liquids have penetrated the housing, or the user or patient may be exposed to electrical shock or faulty readings may appear. Contact your supplier for further action.
- Use of this equipment adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, this equipment and the other equipment should be observed to verify that they are operating normally.

#### **CAUTION:**

- Ensure that all ventilation holes are unblocked to avoid system overheating and false readings.

### **Electrical**

#### **WARNING:**

- Electrical Shock Hazard - Do not remove OPTIS Mobile Next covers. To avoid electrical shock, use only the power cord supplied with the system and connect only to properly grounded wall outlets. Refer to "System Setup" and "Safety Information" for electrical safety information.
- The main power remains switched on when the system is in Standby mode. Avoid direct or indirect (e.g., via the operator) conductive connection between other electrical equipment and the OPTIS Mobile Next. Conductive connection may cause leakage currents to induce ventricular fibrillation. High frequency surgical equipment must not be used on a patient at the same time as PressureWire Guidewire and the OPTIS Mobile Next.

## Warnings and Precautions

---

- Never use a converter adapter to connect the AC plug to an ungrounded wall outlet. Doing so may result in electric shock to the patient or operator and damage to equipment.

### **CAUTION:**

- Do not unplug from AC power or turn off main power until the shutdown is complete, the screens turn black, and the green monitor LEDs turn amber. Disconnecting from AC power before the shutdown is complete may damage the system.

## **Electronic Interference**

### **CAUTION:**

- Radio transmitting equipment, cellular phones, and strong emission sources such as high frequency surgical equipment shall not be used in close proximity to the OPTIS Mobile Next since this could influence the performance of the device.

**Note:** The device should be used in a hospital environment except for near active high frequency (HF) surgical equipment and the radio frequency (RF) shielded room of a medical equipment system for magnetic resonance imaging, where the intensity of electromagnetic (EM) disturbances is high.

## **Aortic Reference Pressure**

### **CAUTION:**

- Check that the monitor cables and aortic pressure transducer (AO) adapter delivered with the OPTIS Mobile Next interface are compatible with the catheterization laboratory system to be used. The AO should be in accordance with ANSI/AAMI BP22-1994. Once the laboratory monitor system has been zeroed, use only the OPTIS Mobile Next to calibrate the AO and PressureWire Guidewire.

## **Defibrillation**

### **CAUTION:**

- The OPTIS Mobile Next is a CF Class I equipment and protected against the effects of a discharge of a defibrillator. PressureWire Guidewire readings may be affected by defibrillation. Recalibrate the PressureWire Guidewire after defibrillation use.

## **System Security**

### **WARNING:**

- To protect the privacy and security of sensitive information, including electronic protected health information (EPHI), and to protect the integrity of the system itself, the system should be located in a physically secure, access-controlled environment. Do not use the OPTIS Mobile Next if there is reason to believe the system's security has been compromised or if the system was unaccounted for during a period of time (i.e., misappropriated, modified, or tampered with).

## System Overview

### System Features

Optical Coherence Tomography (OCT) is an imaging modality that uses fiber-optic technology. The OPTIS™ Mobile Next uses optical imaging catheters that emit near-infrared light to produce high-resolution real-time images.

Fractional Flow Reserve (FFR) is the ratio of distal coronary arterial pressure (Pd) to aortic pressure (Pa), measured during hyperemia. It provides the maximal blood flow in the presence of a stenosis as a fraction of the achievable blood flow that would exist in the hypothetical situation that the stenosis was not present. Pd / Pa at rest is the ratio of distal coronary arterial pressure to aortic pressure measured at resting conditions.

Resting Full-Cycle Ratio (RFR) is the ratio of Pd to Pa at a point in the cardiac cycle where the Pd / Pa ratio is minimal. RFR is designed to be used at rest and, in contrast to Pd / Pa at rest, is a sub-cycle metric.

The physician may use the FFR, Pd / Pa at rest, and RFR parameters, along with knowledge of patient history, medical expertise, and clinical judgment, to determine if therapeutic intervention is indicated.



**CAUTION:** Medical personnel who use the OPTIS Mobile Next software must be aware of the system's limitations. Only operators knowledgeable in OCT and physiologic procedures can determine if use of the OPTIS Mobile Next software and OPTIS Mobile Next are appropriate. Be sure to read Safety Information before operating the OPTIS Mobile Next software for the first time.

---



**CAUTION:** Medical personnel who use the OPTIS Mobile Next must be aware of the system's limitations. Only medical personnel who are knowledgeable in OCT and physiologic procedures can determine if use of the OPTIS Mobile Next is appropriate. Be sure to read Safety Information before operating the OPTIS Mobile Next for the first time.

---

## System Components

The OPTIS Mobile Next includes the following components, integrated into a mobile cart:

- Imaging engine
- Two monitors
- Drive motor and optical controller (DOC)
- Isolation transformer
- Aortic pressure and PressureWire™ Receivers
- Computer, keyboard, mouse
- Power cable

### Note:

- Use only the power cable and accessories provided with the system. Use of other cables or accessories may negatively affect electromagnetic compatibility performance.
- Physiology procedures require a Wi-Box™ AO Transmitter installed in the catheterization laboratory. Contact Abbott Service for more information.
- During installation, the tableside controller (TSC) is customized to operate in a specific room. If the TSC is removed for cleaning or adjustments, it should be returned to the original room.
- If present, the OPTIS™ Connectivity Box (C-Box) is configured to operate in a specific room to simplify integration.



---

**CAUTION:** The above components are integral parts of the OPTIS Mobile Next. The hardware and software must not be modified in any way by the customer. Making such modifications may interfere with correct operation and will void system warranties. Contact an Abbott Technical Service representative for more information.


---

## System Overview

---


### OPTIS Mobile Next - Physician Side

Figure 3. OPTIS Mobile Next - Physician Side

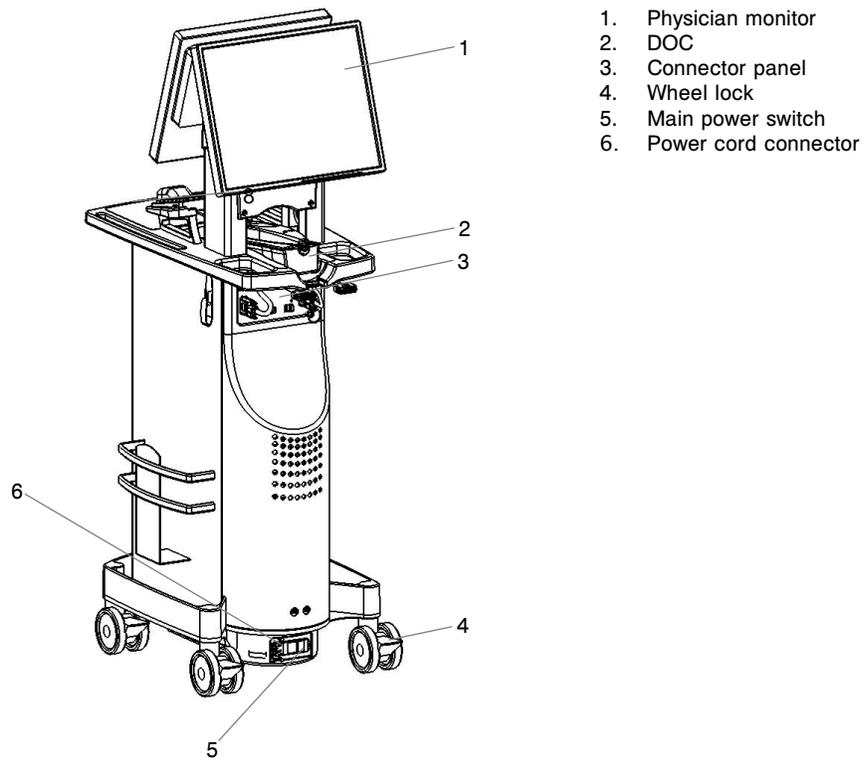

### OPTIS Mobile Next - Operator Side

Figure 4. OPTIS Mobile Next - Operator Side

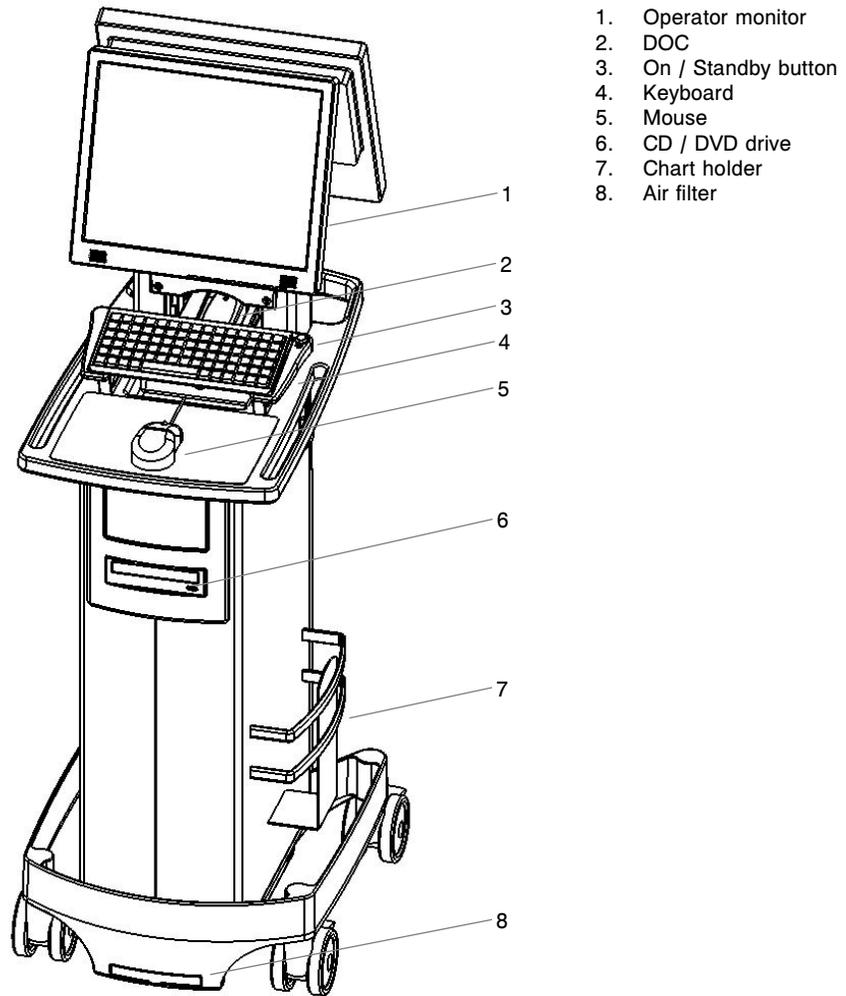


## System Overview

---

### Tablesides Controller (TSC)

Figure 5. Tableside Controller (TSC)

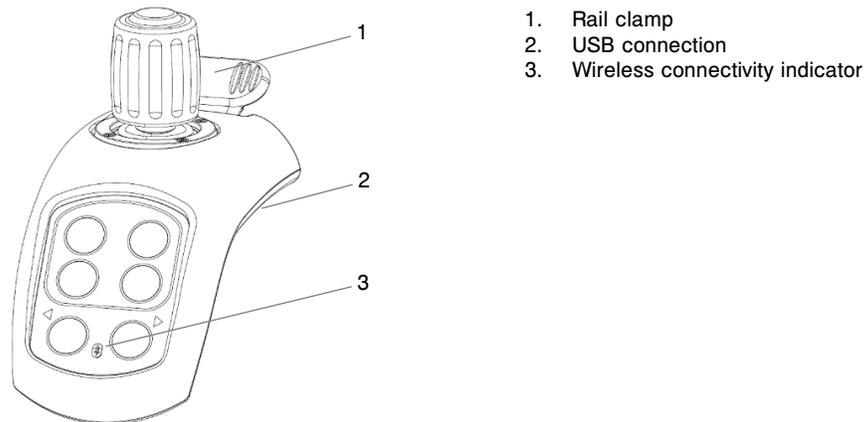

**Note:**

- If the TSC is connected by USB cable, the wireless connectivity indicator does not illuminate.
- Improper handling of the USB connection can damage the port on the connector panel.
- During installation, the TSC is customized to operate in a specific room. If the TSC is removed for cleaning or adjustments, it should be returned to the original room.



---


**CAUTION:** A yellow “no connection” Wireless Connectivity Indicator LED means the tableside controller (TSC) is not connected to the system. Refer to “User Troubleshooting” on page 40 to reconnect.

---

### Drive Motor and Optical Controller (DOC)

The DOC provides bed-side control of the most important OCT imaging functions. Refer to the installed software User Manual for Dragonfly™ Imaging Catheter connection details.

Figure 6. Drive Motor and Optical Controller (DOC)

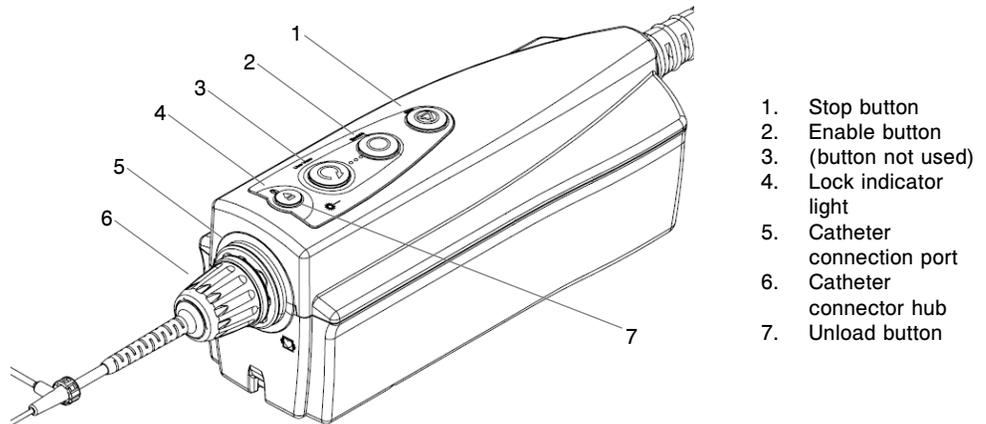


## System Overview

---

### Wi-Box AO Transmitter

The Wi-Box AO Transmitter is installed in the catheterization laboratory between the hemodynamic recording system and the aortic pressure transducer (AO). The position of the Wi-Box AO Transmitter in a catheterization laboratory is shown below.

Figure 7. Wi-Box AO Transmitter in Catheterization Laboratory Configuration

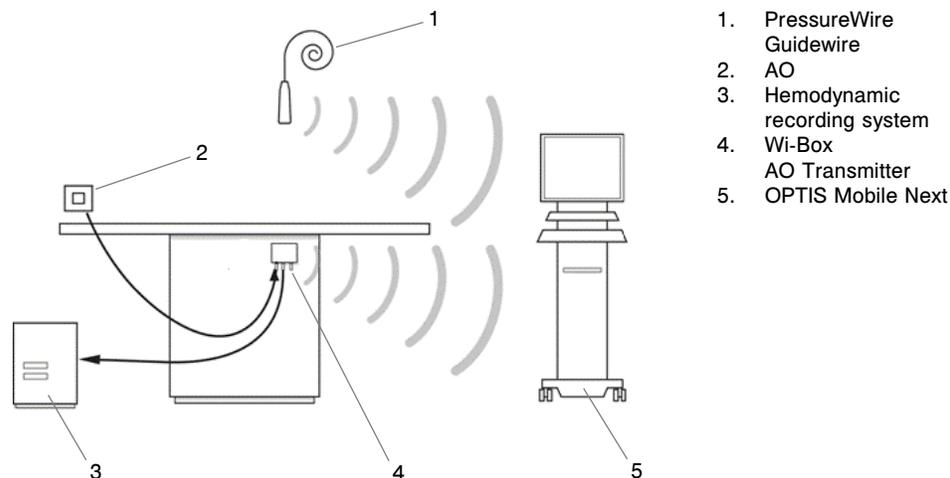

The wireless connection to the Wi-Box AO Transmitter is made during setup for the procedure. Refer to the installed software User Manual for more information.

### System Accessories

- PressureWire Guidewire
- Additional TSCs
- Wi-Box AO Transmitter
- Connectivity box
- Dragonfly™ OPTIS™ Imaging Catheter or Dragonfly OpStar™ Imaging Catheter
- Sterile DOC cover
- 3 ml syringe

**Note:** Contact Abbott Service for order numbers of accessories.

### Spare Parts

- DOC optical connector
- Air filter
- Consumable video cables

## System Setup

### Positioning the System

---



**WARNING:** Failure to position the system as described may lead to a system tipping hazard or a pinching hazard, causing possible patient or operator injury and damage to the system.

---

- Position the OPTIS™ Mobile Next at the foot of the procedure table in a catheterization laboratory with the physician monitor facing the attending physician and not obstructing the boom monitor.

The OPTIS Mobile Next may be placed at other locations; however, care must be taken to ensure the system is clear of any moving equipment, including the angiography system. It is the responsibility of the attending physician to ensure that collisions do not occur.

**Note:** Prior to a procedure, the OPTIS Mobile Next wheels can be left unlocked when it is used near moving equipment. It is recommended that the wheels remain unlocked to allow the system to roll if it is bumped.

---



**CAUTION:** During a procedure, the OPTIS Mobile Next wheels must be locked to avoid any unintended motion of the Dragonfly™ Imaging Catheter.

---

- Mount the TSC onto the procedure table rail in a location that is comfortable for the physician to use during the procedure. Drape the TSC with a protective sterile barrier to maintain sterile technique.
- Ensure that the TSC is in a location that minimizes exposure to fluids.
- Ensure that the power cord and any other connections to the OPTIS Mobile Next are routed to prevent a tripping hazard. Ensure that the main power switch and power plug can be accessed at any time during the procedure.
- Ensure that the OPTIS Mobile Next is positioned so that the connection between the console and the DOC will not be disturbed during use.
- Position the cables to minimize the chance of disconnection.
- If it is required to move the OPTIS Mobile Next, refer to “Moving the System” on page 9.


## System Setup

---

### Attaching and Removing Components (Table Rail)

To attach the TSC to (or remove it from) the patient procedure table rail:

Figure 8. Tableside Controller (TSC)

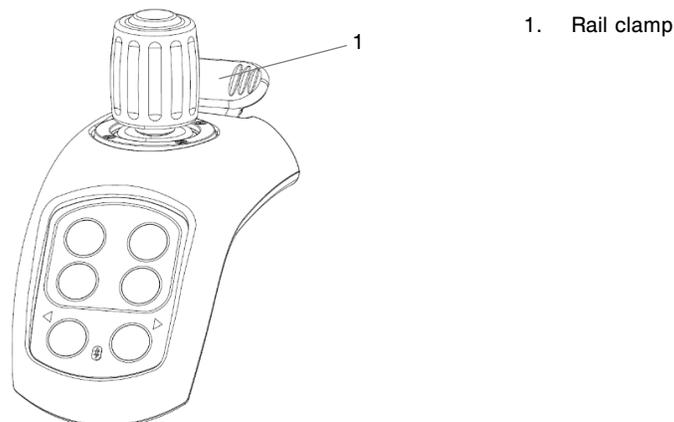

#### Attach

1. Ensure that the clamp is fully open.
2. Place the clamp side of the component onto the rail and continue to hold.
3. Gently push down on the grooved end of the clamp to secure the component onto the rail.
4. Gently test the component to ensure that it is securely fastened to the rail.

**Note:** If a component is moved to a different table, a shim may be required to allow it to clamp properly.

5. Plug the USB cable from the TSC power supply into the bottom of the TSC.



---

**WARNING:** Do not allow the TSC power supply to get wet.

---

#### Remove

1. Unplug the USB cable from the TSC power supply from the bottom of the TSC.
2. Grasp the component from the bottom in one hand (supporting the weight) and lift the grooved end of the clamp to release from the rail.
3. Holding the clamp open, gently pull the component from the rail. To avoid damaging cables, components, or connections that may expose the user to harm, do not drop the component.

## Connecting the System




**WARNING:** All connections to the OPTIS Mobile Next except the TSC in Bluetooth<sup>®</sup> mode must be made through the System Connector Panel. Making connections directly to internal components of the system may bypass isolation features and compromise patient safety.

**Note:** Perform system connections before powering on.

### Power Connector Location

Figure 9. OPTIS Mobile Next Power Connection

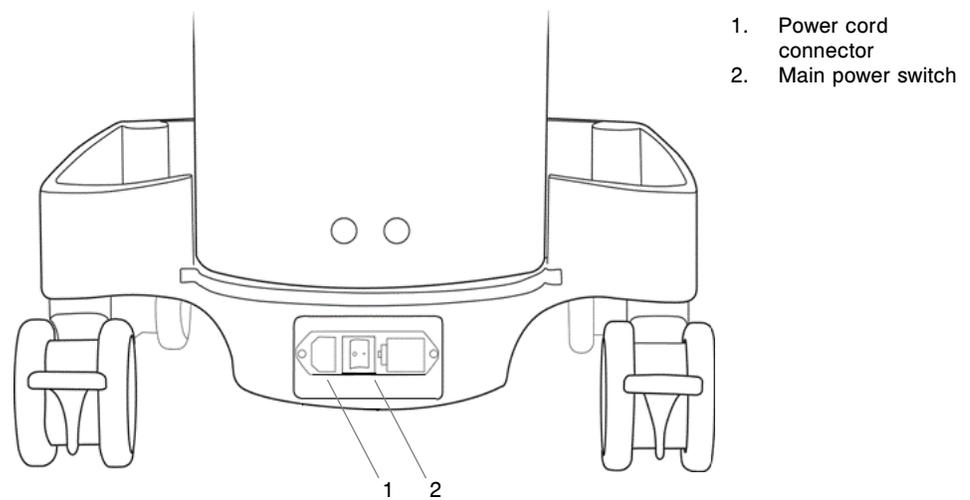

## System Setup

---

### Connecting an External Color Monitor


An external monitor that is capable of displaying a 1280 x 1024 pixel image may be connected to the OPTIS Mobile Next through the video output cable (figure below).



**WARNING:** If the external monitor is being used in the patient vicinity, it must use an isolated power source or it may compromise electrical isolation and cause patient injury.

---

Figure 10. OPTIS Mobile Next Color Monitor Connection

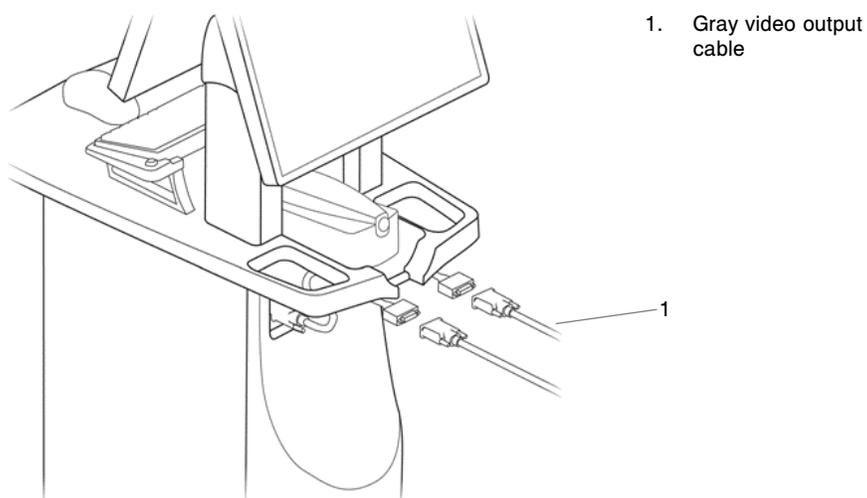


### Connecting X-Ray Video

The OPTIS Mobile Next may be connected to an external x-ray video signal using the video input cable located on the physician side of the device (figure below).

**Note:**

- Video connections at the connector panel should only be removed during preventative maintenance.
- Align the connectors before seating to avoid damaging the connectors.
- Ensure that all connectors are properly seated and thumb screws are fully tightened.

Figure 11. OPTIS Mobile Next X-Ray Video Connection

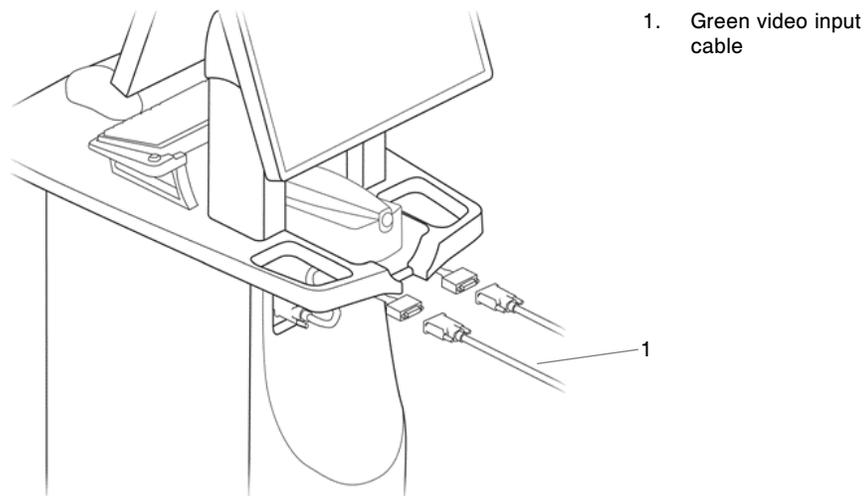

## System Setup

---

### Powering On

For detailed information on electrical requirements, refer to “Making Proper Electrical Connections” on page 11.



---

**WARNING:** Never use a converter adapter to connect the AC plug to an ungrounded wall outlet. Doing so may result in electric shock to the patient or operator and damage to equipment.

---

1. Make sure the power cord is connected to the system and is plugged into a grounded electrical outlet.
2. Secure the power cord using the strain-relief clip on the power cord connector.
3. Turn ON system power by pressing the main power switch at the base of the cart.
4. Confirm that all monitors are powered by observing that the appropriate power indicators are on.
5. Start the system by pressing the On / Standby button located at the upper-right corner of the keyboard. The startup screen appears.
6. The first time the software runs, select a language (if prompted). If necessary, refer to the installed software User Manual to change this selection.
7. The first time the software runs, the End User License Agreement (EULA) displays. Read and agree to the EULA to proceed.
8. Adjust monitor brightness and contrast as necessary.

### Shutting Down



---

**CAUTION:** Do not unplug from AC power or turn off main power until the shutdown is complete, the screens turn black, and the green monitor LEDs turn amber. Disconnecting from AC power before the shutdown is complete may damage the system.

---

**Note:** Use the Shutdown button at the top of the screen to shut down the system. Use of the On / Standby key is not recommended to shut down the system.

1. Click the Shutdown button located at the top of the screen. The system shutdown menu appears.
2. Click Yes to begin the system shutdown, or No to continue using the system.  
If you choose Yes, the computer begins the system shutdown. After 15 seconds, the screens turn black, the green monitor LEDs turn amber, and the system enters Standby mode.
3. After the screens turn black and the green monitor LEDs turn amber, press the main power switch at the base of the cart to turn off system power.
4. If necessary, disconnect the power cord from AC power.

## Cleaning and Maintenance



---

**CAUTION:** Do not perform cleaning or maintenance on the system during a patient case or in the patient environment.

---



---

**CAUTION:** The OPTIS™ Mobile Next accessories should be appropriately classified as a biohazard and disposed of in compliance with applicable facility procedures, local and country laws and regulations. Return the OPTIS Mobile Next to Abbott Medical at the end of its operating life.

---

### Cleaning

The following OPTIS Mobile Next items require cleaning:

- System surfaces
- DOC and DOC optical cable
- TSC
- Connectivity box

### Routine Cleaning Procedure

The OPTIS Mobile Next and TSC should be cleaned following the facility's standard cleaning schedule, or at least every 30 days under normal use.

1. Turn off all system components with accessible power controls and unplug the power cable.
2. Clean system surfaces and the keyboard with a dry cloth, or a dry cloth slightly dampened with water.
3. Clean the LCD surface of the monitor with a lint-free, non-abrasive cloth.



---

**CAUTION:** Do not clean the LCD surface with detergents or other cleaning solutions.

---

4. Clean exposed system cables with a soft cloth moistened with water or a mild detergent.
5. Clean the TSC, DOC, and DOC optical cable with a disinfectant wipe or hypochlorite 1:10 solution and a soft cloth. Be particularly careful not to stress or sharply bend the DOC optical cable.

**Note:**

- Though enclosed in a bag during use, the DOC is the system component most exposed to dirt, fluids, and debris.
  - The TSC and DOC are not waterproof. Be careful not to use excessive moisture when cleaning these devices. Wipe only. Do not soak or spray.
6. Clean all other exposed system cables with a soft cloth moistened with water, or water and a mild detergent.
  7. Clean the air filter on the system as specified in "Air Filter Maintenance Procedure" (page 38).

## Cleaning and Maintenance

---

### Maintenance

#### Contacting Abbott Technical Service

---



**CAUTION:** Only a qualified Abbott Technical Service representative can perform maintenance or service components of the system. Any attempt to open the system components by anyone other than a qualified Abbott Technical Service representative will void the warranty.

---

Service can be contacted at:

Email: OCTservice@abbott.com

Phone (Outside US): +1 651 490 4410

#### Maintenance Procedures

Maintenance of the system consists of:

- Cleaning the optical connection in the DOC and in the Dragonfly™ Imaging Catheter
- Replacing the optical adapter in the DOC
- Cleaning or replacing the air filter
- Inspecting exposed cable connections
- Transferring log files
- Identifying the installed software version

#### Optical Connection Cleaning Procedure

The optical connection between the DOC and the catheter should be cleaned whenever a loss of image quality occurs. Image quality should also be checked every 3 months, and the connection should be cleaned if there is a loss of quality.

---



**CAUTION:** This procedure should not be performed during a patient case on a sterile Dragonfly Imaging Catheter.


---

#### Note:

- Before beginning this procedure, ensure that the Abbott Medical optical fiber connector cleaner is available.
  - Do not touch any of the optical connectors or the end of the optical fiber connector cleaner as this may damage them.
1. If a catheter is connected to the DOC, press the Unload button on the DOC and wait until the "lock" LED stops flashing. When the "lock" LED is off, remove the catheter.
  2. Click the Menu button and select the Setup option. The Setup dialog box displays.

3. Click Service. The Service menu displays.
4. In the DOC Service section of the Service menu, click Enter.
5. The DOC optical carriage moves all the way to the front and locks into position for one minute. Rotation of the DOC rotary motor stops, and the laser source turns off.
6. Remove the sizing cap from the end of the optical fiber connector cleaner (figure below).
7. Insert the cleaner into the center of the optical adapter in the DOC, ensuring that it seats fully, and press until it clicks. The cleaning material in the optical fiber connector cleaner is moved over the optical connection.

Figure 12. Inserting Cleaner into Optical Adapter

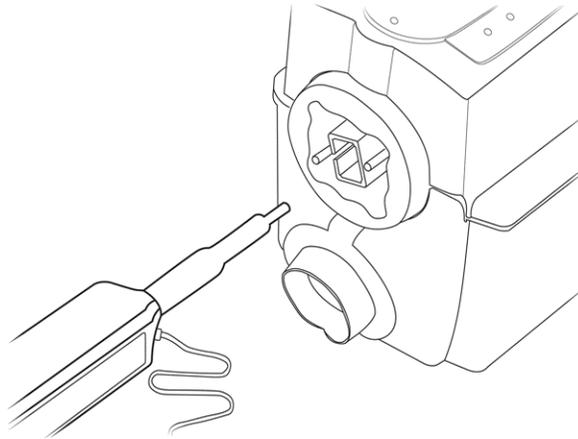


8. Remove the cleaner from the DOC.

## Cleaning and Maintenance

---

9. In the DOC Service section of the Service menu, click Exit. The DOC optical carriage moves all the way to the back and all DOC functions are returned to their normal state.
10. Click OK or Cancel to close the Setup dialog box.
11. Open the sizing cap and place it on the end of the optical fiber connector cleaner (figure below).
12. Insert the cleaner into the optical connection in the catheter, ensuring that it seats fully, and press until it clicks. The cleaning material in the optical fiber connector cleaner is moved over the optical connection.

Figure 13. Inserting Cleaner into Catheter

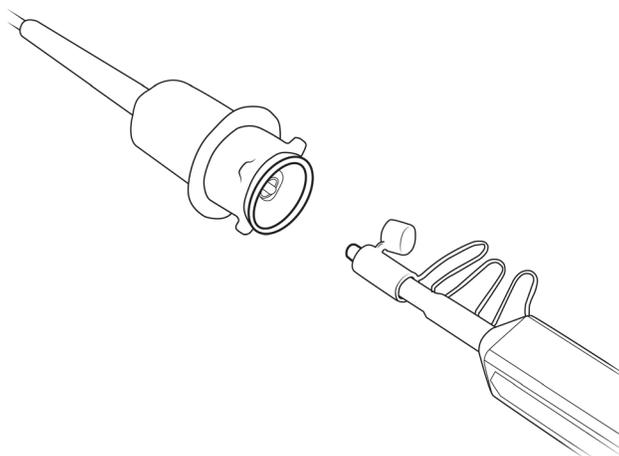

13. Remove the cleaner from the catheter.
14. Reconnect the catheter to the DOC.
15. Return the system to normal operation.

### Optical Adapter Replacement Procedure

The optical adapter should be replaced every 200 cycles or 1 year (whichever occurs first), or if cleaning does not improve image quality. Contact Abbott Service to purchase optical adapters.




**CAUTION:** This procedure should not be performed during a patient case on a sterile Dragonfly Imaging Catheter.

#### Note:

- Before beginning this procedure, ensure that a replacement Abbott Medical optical adapter and supplied pliers are available.
  - Do not touch any of the optical connectors, as this may damage them.
1. If a catheter is connected to the DOC, press the Unload button on the DOC and wait until the "lock" LED stops flashing. When the "lock" LED is off, remove the catheter.
  2. Click the Menu button and select the Setup option. The Setup dialog box displays.
  3. Click Service. The Service menu displays.
  4. In the DOC Service section of the Service menu, click Enter. The DOC optical carriage moves all the way to the front and locks into position for one minute. Rotation of the DOC rotary motor stops and the laser source turns off.
  5. Use pliers to grip either short surface of the adapter as shown (figure below). Ensure that the pliers seat over the lip on the end of the adapter.

Figure 14. Proper Gripping of Adapter for Removal

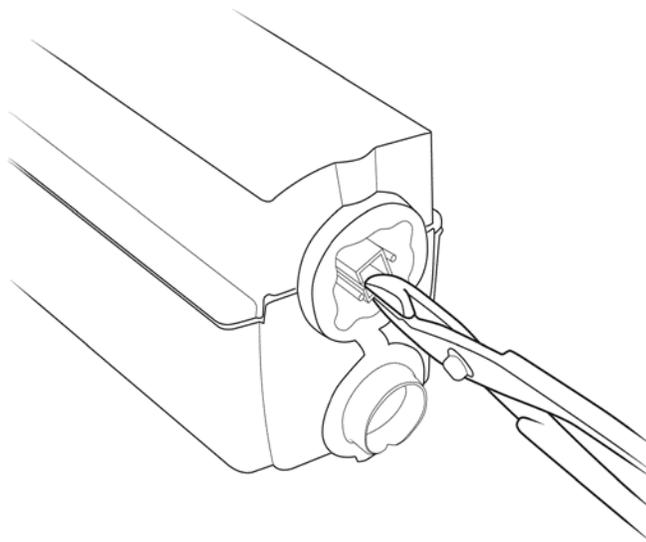


## Cleaning and Maintenance

---

6. Pull the adapter straight out of the DOC.  
**Note:** Ensure that the adapter does not rotate while it is being removed, as this could damage the DOC or break the adapter.
7. Remove the cap and plug from the replacement optical adapter.  
**Note:** Do not touch any of the optical connectors, as this may damage them.
8. Using fingers, align the new adapter with the DOC, ensuring that the key is aligned with the slot in the optical carriage, and firmly press it into place. An audible click is produced when the adapter seats.  
**Note:** If the carriage moves when you press on the adapter, click the Exit button in the DOC Service section of the Service menu. When it changes to Enter, click it again. When the optical carriage is locked into position at the front of the DOC, firmly press the adapter into place.

Figure 15. Alignment of Optical Adapter with Optical Carriage

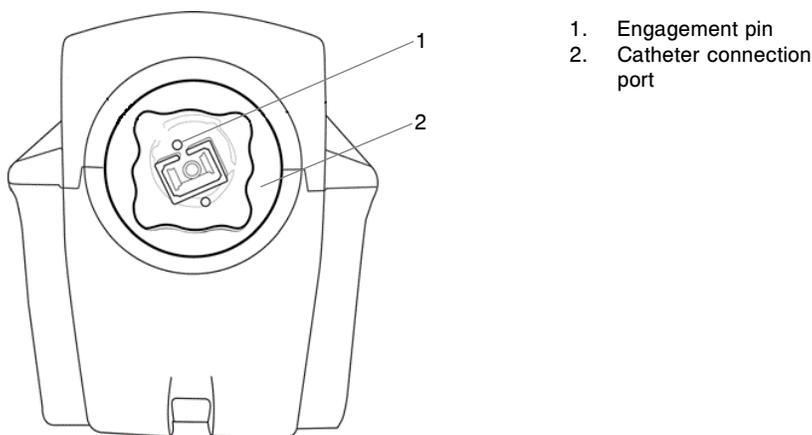

9. In the DOC Service section of the Service menu, click Exit. The DOC optical carriage moves all the way to the back and restores all DOC functions to their normal state.
10. Click OK or Cancel to close the Setup dialog box.
11. Return the system to normal operation.

### Air Filter Maintenance Procedure

The air filter should be cleaned every six months under normal use. If necessary, contact Abbott Service to purchase air filters.

1. Locate the air filter holder at the bottom of the cart (refer to the Operator Side figure in “System Components” on page 21).
2. Pull the filter holder out of the cart base.
3. Remove the filter and brush or vacuum off dust (replace if necessary).
4. Place the filter into the filter holder.
5. Push the filter holder back into the cart base.

### **Cable Connection Inspection Procedure**

1. Ensure that the power connection to the system is fully seated and secured with the strain-relief clip.
2. If a secondary ground connection is being used, ensure that both ends of the cable are secure.
3. Ensure that all other connectors are fully seated and properly secured.

### **Consumable Video Connector Replacement Procedure**

The boom monitor and angiographic DVI cables (available from Abbott) use consumable adapters that should be replaced every 200 cycles.

1. Turn off the OPTIS Mobile Next power.
2. Disconnect the consumable DVI cable from the back of the OPTIS Mobile Next or disconnect the consumable adapter from the video cable.
3. Connect the new DVI cable or adapter.
4. Properly seat all connectors and fully tighten all thumb screws.

### **Infection Control**

Follow the infection control procedures established in your institution for protection of both staff and patient.

Blood on system components, panels, and cables should be removed by using a gauze pad with soap and water, and drying with a soft cloth to prevent corrosion. The DOC cable can be cleaned with a disinfectant wipe or hypochlorite 1:10 solution and a soft cloth.

## Cleaning and Maintenance

---

### User Troubleshooting

The table below provides basic guidelines for troubleshooting the OPTIS Mobile Next. Refer to the installed software User Manual for additional troubleshooting procedures.

If the problem is not resolved after attempting the suggested remedies, contact Abbott Service or email [OCTservice@abbott.com](mailto:OCTservice@abbott.com).

Table 1. User Troubleshooting Tips

Symptom	Possible Causes	Remedy
<b>General</b>		
Screen blank, power indicator on monitor not lit.	Display not turned on.	Press the power button on the monitor to turn on monitor power.
	Display power cord unplugged.	Plug the monitor power cord into the back of monitor.
	System power not turned on.	Turn on the system power with the main power switch, located next to the power cord connection.
	System power cord not plugged in or not tight at either system end or wall connection.	Check to make sure plug is tightly connected to both the system and the wall outlet.
	Main system power fuse is blown.	Refer to the Electrical label on the system (located next to the power cord connection) for fuse information. Contact Abbott Service for instructions.
	Outlet power disrupted.	Check voltage at the wall outlet.
Screen blank, power indicator on monitor lit.	PC auto boot failed.	Turn off the main power switch and wait fifteen seconds. Turn the main power switch back on and press the On / Standby button on the right side of the keyboard to start the system. If the system still does not start, contact Abbott Service for instructions.
	Monitor not enabled.	Click <Alt+C> on the keyboard to enable the display. If the screen remains blank, turn off the main power switch and wait fifteen seconds. Turn the main power switch back on and press the On / Standby button on the right side of the keyboard to start the system.
<b>Connections</b>		
During data export, the system does not list the USB drive plugged into the USB port.	The connected USB drive is not compatible with the system, or the USB drive requires formatting.	Connect only a USB Drive supported by Windows 10 OS. Refer to the Instructions for Use that came with the USB drive to determine if formatting is required.
Screen message "Imaging engine initialization failed" is displayed at startup.	This message can be caused by several problems, including loose or damaged system connections.	Shut down the system, turn off the main system power, and wait 15 seconds. Then turn the system back on. If the error is displayed again, contact Abbott Service for instructions.
<b>DOC</b>		
DOC makes excessive noise without imaging catheter connected.	DOC mechanism failure.	Contact Abbott Service to obtain a replacement DOC.

## Cleaning and Maintenance

Table 1. User Troubleshooting Tips (continued)

Symptom	Possible Causes	Remedy
<b>Imaging</b>		
OCT image dim, with no background noise visible.	Monitor contrast and brightness set incorrectly.	Set monitor contrast and brightness using monitor controls.
	Image contrast levels set incorrectly.	Check the Presentation Settings on the Settings tab of the OCT Settings menu (normal settings are: Black level = 5%, White level = 90%). With the optical fiber rotating (scanning mode), reduce the Black level until background noise just becomes visible. Lack of background noise during optical fiber rotation indicates a defective imaging engine. See other possible causes and remedies below.
	Defective imaging catheter causing system saturation.	Remove imaging catheter from DOC. If background noise appears, the imaging catheter is defective. Replace catheter.
	Dirty connection between DOC and imaging catheter.	Refer to "Optical Connection Cleaning Procedure" on page 34 to clean the connection.
<b>Tablesides Controller</b>		
Wireless Connectivity Indicator LED illuminates yellow color.	No wireless connection to tablesides controller.	<p>Click Menu / Setup. Select Room Manager. Ensure the tablesides controller is added as a wireless device and the serial number displayed matches the device serial number on back label.</p> <p>If the serial numbers match and the wireless connectivity Indicator LED on the tablesides controller remains yellow, reconnect the tablesides controller as follows:</p> <p>Remove the tablesides controller device by clicking the Remove button. After successful removal, click the Add button to add the tablesides controller device.</p>

## System Disposal

Disposal of the equipment must be in accordance with local laws.

## System Specifications

### System - Safety and Regulatory

Table 2. System Safety and Regulatory Specifications

Category	Specifications
Regulatory Approvals	<p>US 510(k) clearance</p> <p style="font-size: 24pt; font-weight: bold;">CE2797</p> <p>European conformity, affixed according to the relevant provisions of EU MDR 2017/745 and 2011/65/EU, and RED directive 2014/53/EU Annex II. Hereby, Abbott Medical declares that this device complies with the essential requirements and other relevant provisions of these directives.</p> <p>The OPTIS Mobile Next complies with FDA performance standards for laser products except for deviations pursuant to laser Notice No. 50, dated June 24, 2007.</p> <p>Abbott Medical hereby declares that OPTIS Mobile Next is in compliance with the essential requirements and other relevant provisions of EU MDR 2017/745, 2011/65/EU, and RED directive 2014/53/EU. A copy of the Full Declaration of Conformity can be obtained by contacting the EU Representative.</p>
Safety Standards	<p>IEC 60601-1:2005/A1:2012 (per Annex ZZ) Medical electrical equipment Part 1: General requirements for basic safety and essential performance</p> <p>CAN/CSA C22.2 No. 60601-1:2008, Medical electrical equipment Part 1: General requirements for basic safety and essential performance</p> <p>IEC 60825-1, 3rd Ed., 2014 Safety of Laser Products Part 1: Equipment classification and requirements</p> <p>IEC 60601-1-2:2014 Ed.4 Medical electrical equipment - Part 1-2: General requirements for basic safety and essential performance - Collateral standard: Electromagnetic compatibility - Requirements and tests – Group 1 Equipment, Class A</p> <p>ANSI/AAMI ES60601-1:2005/(R)2012, Medical electrical equipment, Part 1: General requirements for basic safety and essential performance</p>
Environmental	<p>RoHS Directive 2011/65/EU</p> <p>REACH Directive EC 1907/2006</p> <p>WEEE Directive 2012/19/EU</p>
Electromagnetic Compatibility (EMC)	Refer to Electromagnetic Emission and Electromagnetic Immunity for detailed specifications.
<b>Classifications</b>	
Type of Protection, Shock	Class 1
Degree of Protection, Shock	Type CF DOC with catheter (CF label at DOC cable exit on Connector Panel)
Degree of Protection, Ingress	Console - IPX0 DOC - IPX0, use with Sterile DOC cover for ingress protection Tablesides Controller - IPX3 Connectivity Box - IPX0
Method of Disinfection	Console and DOC will withstand without damage or deterioration disinfection by wiping with a hypochlorite 1:10 solution.
Flammable Mixtures	Not for use in presence of flammable anesthetic mixture with air or with oxygen or nitrous oxide.
Mode of Operation	Continuous

## System Specifications

Table 2. System Safety and Regulatory Specifications (continued)

Category	Specifications
<b>Leakage and Auxiliary Current</b>	
Chassis Leakage Current	< 100 $\mu$ a rms normal condition < 500 $\mu$ a rms single-fault condition
Patient Leakage Current	Measured at patient end of DOC: < 10 $\mu$ a rms normal condition < 50 $\mu$ a rms single-fault condition

## System - Electrical and Physical

Table 3. System Electrical and Physical Specifications

Parameter	Specification
<b>Power Input</b>	
Line Voltage	100/120/220/240 VAC $\pm$ 10%, user selectable 50/60 Hz $\pm$ 1 Hz
Power Consumption	Active: < 400 VA Standby: < 30 VA
<b>Radio Specifications</b>	
<b>Drive Motor and Optical Controller (DOC)</b>	
Frequency Range	13.553 - 13.567 MHz (ISM-band)
Type	Amplitude-Shift Keying (ASK)
Radiated Power	Effective Radiated Power (ERP):-43.05 dBm
<b>Tableside Controller (TSC)</b>	
Frequency Range	2.400 - 2.4835 GHz (ISM-band)
Type	GFSK, DQPSK, 8-DPSK
Radiated Power	Bluetooth <sup>†</sup> power Class 2
<b>Input-Output Panel Bluetooth<sup>†</sup> Adapter</b>	
Frequency Range	2.4 - 2.48 GHz (ISM-band)
Type	GFSK, DQPSK, 8-DPSK
Radiated Power	Bluetooth <sup>†</sup> power Class 1
<b>FFR Receivers</b>	
Frequency Range	2.4 - 2.4835 GHz (ISM-band)
Type	Frequency hopping spread spectrum (FHSS)
Range	Up to 4 m  <b>Note:</b> Radio range is reduced by objects and walls. Keep Transmitter and receiver in line of sight wherever possible.
Delay Time	<20 ms
<b>Transport and Storage Conditions (permissible ranges)</b>	
Ambient Temperature	-20 to +50 degrees C
Relative Humidity	25% - 90%, non-condensing
<b>Operating Conditions</b>	
Ambient Temperature	+10 to +32 degrees C
Relative Humidity	30% to 85%, non-condensing
<b>Mechanical Specifications</b>	
Weight	80 kg (176 lbs) max with all accessories
Overall Dimensions	145 cm H x 61 cm W x 71 cm D $\pm$ 5 mm

## System Specifications

Table 3. System Electrical and Physical Specifications (continued)

Parameter	Specification
Mechanical Specifications - TSC	
Weight	1.5 lbs (0.7 kg)
Overall Dimensions	21 x 9 x 14 cm
Lifetime of Device	
Device Life (System)	1000 cases minimum (385 cases / yr., $\geq 2$ yrs.)

## Imaging Specifications

Table 4. Imaging Specifications

Parameter	Specification
Optical Parameters - Measured at System Aperture (DOC Optical Port)	
Scanning Laser Source Optical Power	22.6 mW maximum @ 1305 nm $\pm$ 55 nm (Class 1M Laser Output per IEC 60825-1)
Visible Laser Optical Power	1.45 mW maximum @ 670 nm $\pm$ 30 nm (nominal) (Class 1M Laser Output per IEC 60825-1)
Pullback Parameters	
Pullback Range	54 mm, 75 mm
Pullback Speed Settings	18.0 mm/sec, 36.0 mm/sec
General Scan Parameters	
A-Scan Range in Air	7.0 mm
A-Scan Range in Contrast	4.83 mm
Diameter Measurement Accuracy	7% $\pm$ 0.1 mm
Area Measurement Accuracy	10% $\pm$ 0.1 mm <sup>2</sup>
Axial Resolution	$\leq 20$ $\mu$ m in tissue
Optical Sensitivity	100 dB minimum
A-Scans per Second	81 kHz minimum
Frame Rate	180 frames/second (Hz)

## Physiology Specifications

Table 5. Physiology Specifications

Parameter	Specification
Aortic Pressure Transducer Pressure (Wi-Box™ AO Transmitter to OPTIS™ Mobile Next)	
Operating pressure	-200 to +450 mm Hg
Accuracy	$\pm 1$ mm Hg or $\pm 1\%$ of reading, whichever is greater
PW Pressure	
Operating pressure	-30 to +300 mm Hg
Accuracy	$\pm 1$ mm Hg plus $\pm 1\%$ of reading (-30 to 50 mm Hg) $\pm 3\%$ of reading (50 to 300 mm Hg)
Aortic Pressure Transducer Pressure (Wi-Box to hemodynamic recording system)	
Direct galvanic connection	
Max pressure shift	<2 mm Hg

## Electromagnetic Emissions

Table 6. Guidance and Manufacturer's Declaration - Electromagnetic Emissions

The OPTIS Mobile Next is intended for use in the electromagnetic environment specified below. The customer or user of the OPTIS Mobile Next should ensure that it is used in such an environment.

Emissions Test	Compliance	Electromagnetic Environment Guidance
RF emissions CISPR 11	Group 1	The OPTIS Mobile Next uses RF energy only for its internal function. Therefore, its RF emissions are very low and not likely to cause any interference with nearby electronic equipment.
RF emissions CISPR 11	Class A	The emission characteristics of the OPTIS Mobile Next are suitable for use in industrial areas and hospitals (CISPR 11 class A). System should not be used in a residential (domestic) environment (CISPR 11 class B is required in support of domestic use).
Harmonic emissions IEC 61000-3-2	Class A	
Voltage fluctuations / flicker emissions IEC-61000-3-3	Complies	

**Note:** The emission characteristics of this equipment make it suitable for use in industrial areas and hospitals (CISPR 11 class A). If it is used in a residential environment (for which CISPR 11 class B is normally required), this equipment might not offer adequate protection to radio-frequency communication services. The user might need to take mitigation measures, such as relocating or re-orienting the equipment.

## Electromagnetic Immunity

Table 7. Guidance and Manufacturer's Declaration - Electromagnetic Immunity

The device is intended for use in the electromagnetic environment specified below. The customer or the user of the device should ensure that it is used in such an environment.

Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment - Guidance
Electrostatic discharge (ESD) EN 61000-4-2 (IEC 61000-4-2)	±8 kV contact ±15 kV air	±8 kV contact ±15 kV air	Floors should be wood, concrete, or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient / burst EN 61000-4-4 (IEC 61000-4-4)	±2 kV for power supply lines ±1 kV for input / output lines	±2 kV ±1 kV	Mains power quality should be that of a typical commercial or hospital environment.
Surge EN 61000-4-5 (IEC 61000-4-5)	±1 kV differential mode ±2 kV common mode	±1 kV ±2 kV	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions, and voltage variation on power supply input lines. IEC 61000-4-11	0% $U_T$ ; 0.5 cycle At 0°, 45°, 90°, 135°, 180°, 225°, 270° and 315° 0% $U_T$ ; 1 cycle and 70% $U_T$ ; 25/30 cycles Single phase: at 0° 0% $U_T$ ; for 5 sec @ 60 Hz (300 cycles) 0% $U_T$ ; 250/300 cycles	100% dropout in VNOM for 0.5 cycle at listed phase angles 100% dropout in VNOM for 1 cycle at 0° 30% dropout in VNOM for 25/30 cycles at 0° 100% dropout in VNOM for 5 sec 100% interrupt in VNOM for 250/300 cycles	Mains power quality should be that of a typical commercial or hospital environment. If the user of the device requires continued operation during power mains interruptions, it is recommended that the device be powered from an uninterruptible power supply or a battery.

## System Specifications

Table 7 (continued). Guidance and Manufacturer's Declaration - Electromagnetic Immunity

The device is intended for use in the electromagnetic environment specified below. The customer or the user of the device should ensure that it is used in such an environment.

Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment - Guidance
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	30 A/m	30 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.

**Note:**  $U_T$  is the AC mains voltage prior to application of the test level.

Table 8. Guidance and Manufacturer's Declaration - Electromagnetic Immunity

The device is intended for use in the electromagnetic environment specified below. The customer or the user of the device should ensure that it is used in such an environment.

Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment - Guidance
Conducted RF IEC 61000-4-6	3 Vrms 150 kHz to 80 MHz	3 Vrms [ $V_1 = 3$ ]	Portable and mobile RF communications equipment should be used no closer to any part of the device, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the Transmitter. Recommended separation distance $d = \left[ \frac{3.5}{V_1} \right] \sqrt{P}$ $d = [1.2] \sqrt{P}$
Radiated RF IEC 61000-4-3	3 V/m 80 MHz to 2.7 GHz	3 V/m [ $E_1 = 3$ ]	80 MHz to 800 MHz $d = \left[ \frac{3.5}{E_1} \right] \sqrt{P}$ $d = [1.2] \sqrt{P}$ 800 MHz to 2.7 GHz $d = \left[ \frac{7}{E_1} \right] \sqrt{P}$ $d = [2.3] \sqrt{P}$ where $P$ is the maximum output power rating of the Transmitter in watts (W) according to the Transmitter manufacturer and $d$ is the recommended separation distance in meters (m) Field strengths from fixed RF Transmitters, as determined by an electromagnetic site survey, <sup>a</sup> should be less than the compliance level in each frequency range. <sup>b</sup> Interference may occur in the vicinity of equipment marked with the following symbol: 
Immunity to Proximity Fields from RF wireless communications equipment IEC 60601-1-2 (Clause 8.10)	385-5785 MHz	9-28 V/m	Per IEC 60601-1-2 (Per Table 9 of Standard)

## System Specifications

Table 8 (continued). Guidance and Manufacturer's Declaration - Electromagnetic Immunity

The device is intended for use in the electromagnetic environment specified below. The customer or the user of the device should ensure that it is used in such an environment.

**Note:** At 80 MHz and 800 MHz, the higher frequency range applies.

**Note:** These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.

- a Field strengths from fixed Transmitters, such as base stations for radio (cellular / cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast, and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF Transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the device is used exceeds the applicable RF compliance level above, the device should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the device.
- b Over the frequency range 150 kHz to 80 MHz, field strengths should be less than  $[V_1]$  V/m.

## Recommended Separation Distances

Table 9. Recommended separation distances between portable and mobile RF communications equipment and the OPTIS™ Mobile Next

The OPTIS Mobile Next is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the OPTIS Mobile Next can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the OPTIS Mobile Next as recommended below, according to the maximum output power of the communications equipment.

Rated maximum output power of Transmitter W	Separation distance according to frequency of Transmitter m		
	150 kHz to 80 MHz $d=1.2\sqrt{P}$	80 MHz to 800 MHz $d=1.2\sqrt{P}$	800 MHz to 2.7 GHz $d=2.3\sqrt{P}$
0.01	0.12	0.12	0.23
0.1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3

For transmitters rated at a maximum output power not listed above, the recommended separation distance  $d$  in meters (m) can be estimated using the equation applicable to the frequency of the transmitter, where  $P$  is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

**Note:** At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

**Note:** These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.

## System Specifications

---

### FCC Statement

This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.

Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Changes or modifications not expressly approved by Abbott Medical could void the user's authority to operate the equipment.

### Essential Performance

#### Imaging

Will compute the diameter of a lumen:

- Accuracy of measurements presented must meet Product Requirements specified in the Design History File (DHF).
- The lumen must be displayed on the screen.

Will compute the length of a lumen:

- Accuracy of measurements presented must meet Product Requirements specified in the DHF.
- The lumen must be displayed on the screen.

#### Physiology

Pressure measurement and ratio display:

- Accuracy of measurements presented must meet Product Requirements specified in the DHF.

Reference Abbott website for patent markings: [www.abbott.com/patents](http://www.abbott.com/patents)

<sup>™</sup> Indicates a trademark of the Abbott group of companies.

‡ Indicates a third-party trademark, which is property of its respective owner.

© 2021 Abbott. All Rights Reserved.





**Abbott Medical**  
4 Robbins Road  
Westford, MA 01886 USA  
TEL: (855) 478-5833  
Outside USA TEL: +1 651-756-5833



**EC REP Abbott Medical**  
The Corporate Village  
Da Vincilaan 11 Box F1  
1935 Zaventem  
Belgium  
TEL: +32 2 774 68 11

2021-02  
ARTEN600173816 A



ARTEN600173816

